

NSLS-II Vacuum Control for Chamber Acceptance

*H. Xu, L.R. Dalesio, M. Ferreira, D. T. Zigrosser, H. Hseuh,
Photon Science Directorate, BNL, Upton, NY 11973, U.S.A.*

WEPKN018



Photon Sciences



Abstract: The National Synchrotron Light Source II (NSLS-II) uses extruded aluminium chambers as an integral part of the vacuum system. Prior to installation in the Storage Ring all dipole and multipole chamber assemblies must be tested to ensure vacuum integrity. A significant part of the chamber test requires a full bakeout of the assembly, as well as control and monitoring of the titanium sublimation pumps (TSP), non-evaporable getter pumps (NEG) and ion pumps. Data that will be acquired by the system during bakeouts includes system temperature, vacuum pressure, residual gas analyzer (RGA) scans, ion pump current, TSP operation and NEG activation. This data will be used as part of the acceptance process of the chambers prior to the installation in the storage ring tunnel. This paper presents the design and implementation of the vacuum bakeout control, as well as related vacuum control issues.

INTRODUCTION

The NSLS-II storage ring is made up of 30 cells and 30 straight sections. Each vacuum cell consists of five basic chambers; an upstream matching multipole chamber, a dipole chamber, a high dispersion section multipole chamber, a second dipole chamber, and a downstream matching multipole chamber. There are RF-shielded bellows connecting these chambers together. The straight sections, either 6.6 m or 9.3 m long between the cells are for insertion devices and for special sub-systems such as RF cavities, injection devices, , and so forth. Most of the NSLS-II storage vacuum chambers are made of extruded aluminium with specific cross-sections. These vacuum chambers allow in-situ bakeouts to 150°C to help remove absorbents, such as water, and contaminants on the inner surface.

VACUUM CHAMBER BAKEOUTS

The vacuum chambers undergo at least two bakeout cycles prior to their installation in the storage ring. Once the chambers are instrumented with vacuum components such as NEG strips, small ion pump, gauging and RGA, they are prepped for the first vacuum bakeout. The second vacuum bakeout occurs at the end of girder integration, after the installation and alignment of the magnets and chambers on the girder assembly, and with the integration of peripheral components, such as large ion pumps, TSP, NEG strips, photon absorbers, and vacuum gauges. The final bakeout will be carried out in storage ring tunnel after the installation and alignment of individual chamber/magnet girders in the tunnel, the connection of the five girder chambers with RF shielded bellows and the mounting of the RF shielded gate valves at the ends of the cell. It's planned to take a similar approach to the bakeout of an entire cell in the storage ring. This paper focuses on girder bakeouts.



Figure 1: Typical NSLS-II girder assembly

VACUUM GIRDER ASSEMBLY BAKEOUT

Each girder assembly is divided into several bakeout zones. All heating zones are controlled by a multiple zone bakeout system, a BNL design incorporating 12 or 24 Omega signal zone temperature controllers with solid state relays housed in a common chassis. Over temperature interlocks are provided to protect chamber assemblies from overheating. The vacuum chamber is pumped down with a turbomolecular pump backed by a dry mechanical pump during the bakeout. The vacuum level and gas composition are monitored continuously using vacuum gauges and RGA during the bakeout. A ~ 2.5 hour ramp period is programmed to reach the designed temperature value. The entire vacuum chamber is then held at 150°C for ~12 hours to remove absorbed water and other contaminants from the surfaces. The sputter ion pumps, titanium sublimation pumps, and NEG strips are degassed during the soak period.

Table1: Typical vacuum components and controllers of girder bakeout system

| | |
|---|---|
| Cold Cathode Gauge (CCG) | 2 |
| Convection Pirani Gauge (TCG) | 1 |
| Vacuum Gauge Controller (VGC) | 1 |
| Sputter Ion Pump (IP) | 2 |
| Ion Pump Controller (IPC) | 1 |
| Titanium Sublimation Pump (TSP) | 1 |
| Titanium Sublimation Pump Controller (TSPC) | 1 |
| Non-Evaporable Getter Strip (NEG) | 1 |
| DC Power Supply for NEG Strip | 1 |
| Bakeout Cart (BC) | 1 |
| Residual Gas Analyzer (RGA) | 1 |
| Turbomolecular Pump Station (TMP) | 1 |
| I/O Controller | 1 |
| Data Server | 1 |
| Uninterruptible Power Supply(UPS) | 1 |

CONTROL FOR CHAMBER BAKING

Overview

Figure 2 shows the architecture of the EPICS based vacuum bakeout control system.

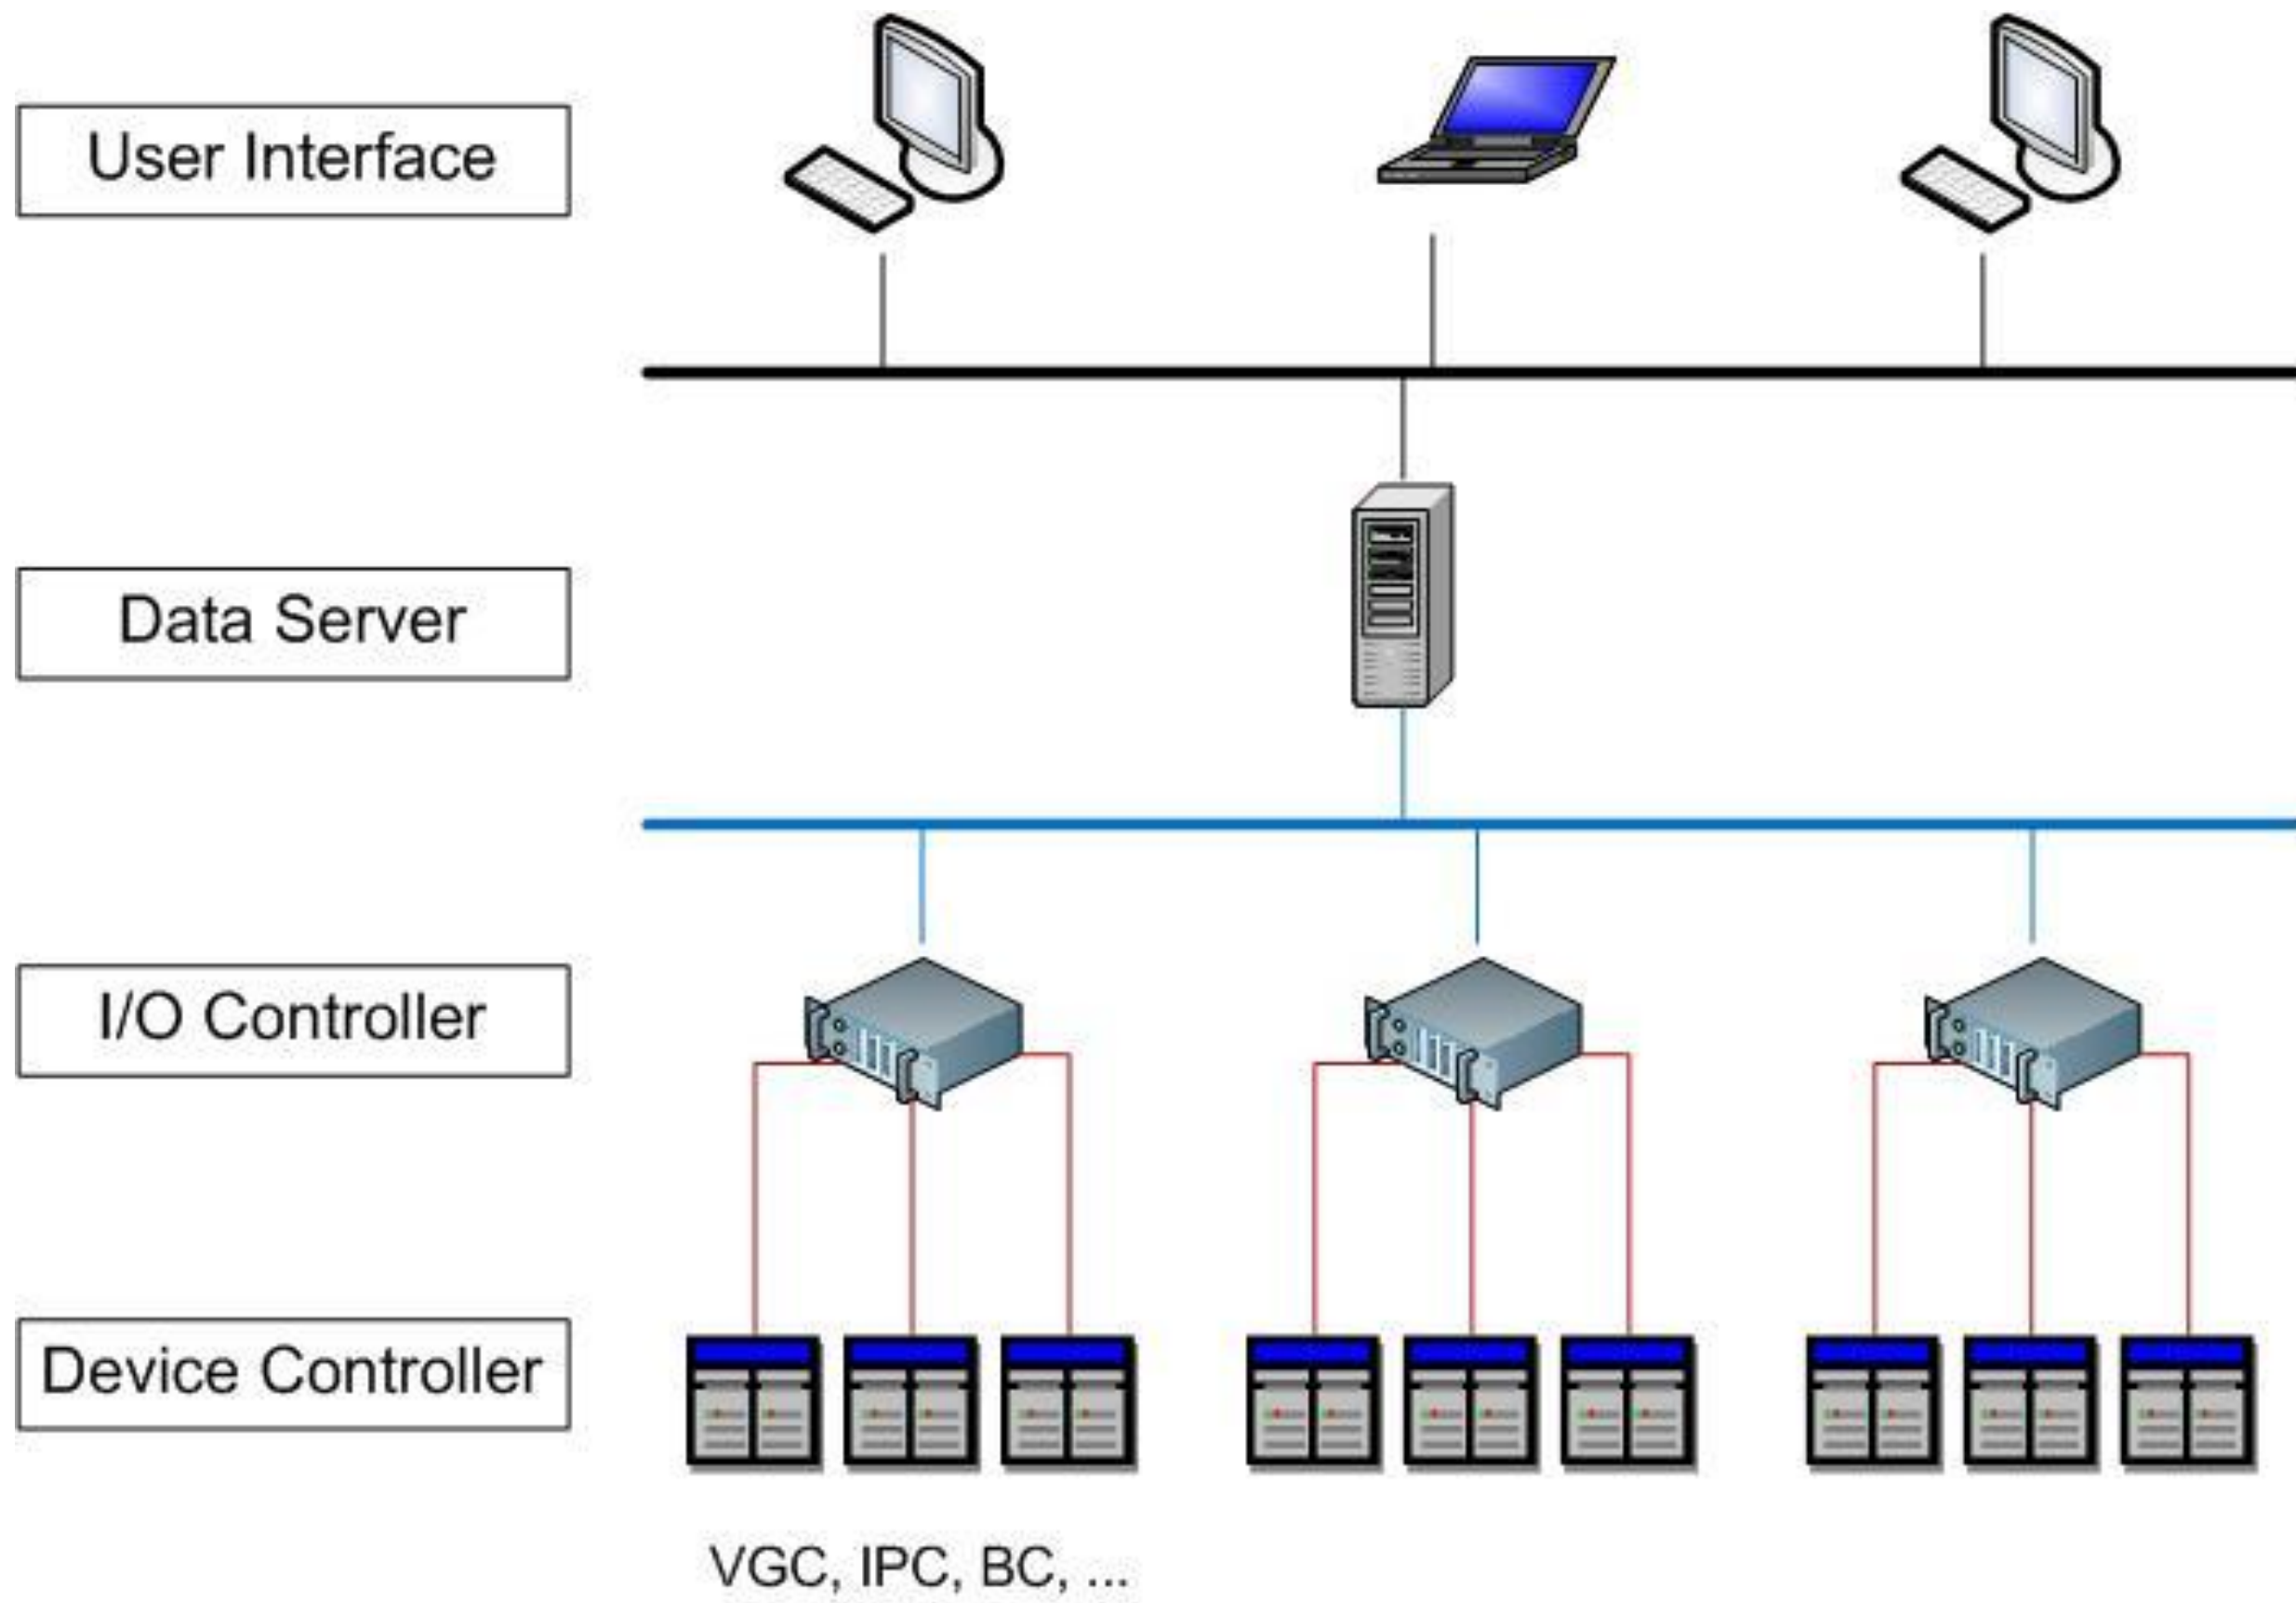


Figure 2: Control architecture for girder assembly bakeout

IOC

Considering that the parameters to be monitored and controlled are much less than 1000 for girder bakeout system, we adopted soft IOC which runs on a Moxa DA-710. The Moxa works as both the IOC and terminal server. The DA-710 is based on the Intel x86 processor and runs on pre-installed Linux platform. It comes with 4 PCI slots for expansion modules and supports up to 32 serial ports.

Operator Interface

All of the monitor and control panels are created with software tools in Control System Studio (CSS). A user-friendly interface was developed based on working experience with vacuum operators and engineers. The interface allows the operators to edit the desired ramp/soak profiles and provides the option to use predefined recipes. All zone temperatures, and gauge pressure readings are shown on main display panel. All zone temperatures, and gauge pressure readings are shown on main display panel as shown in Figure 3.

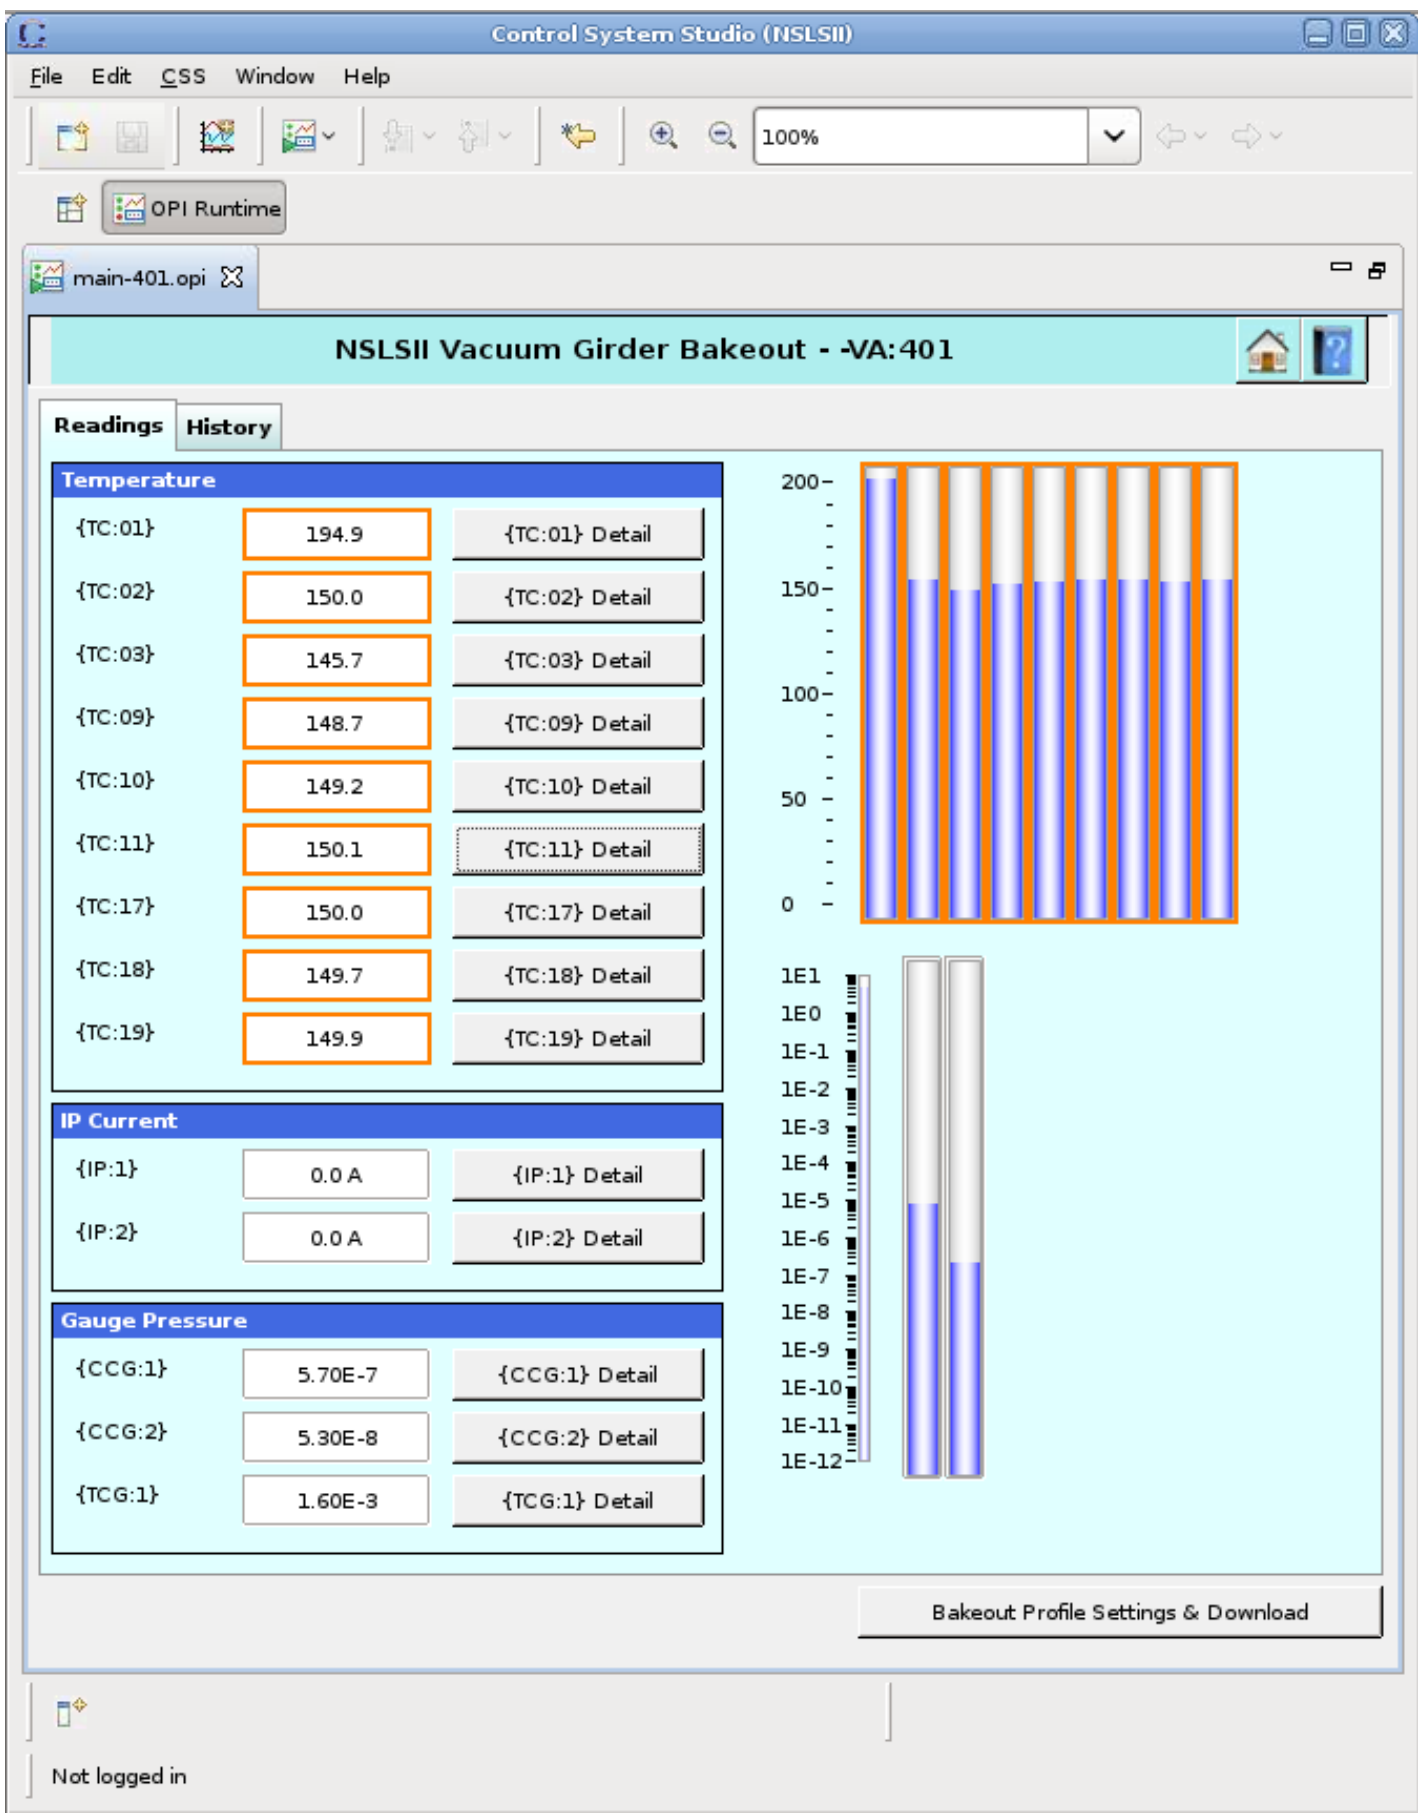


Figure 3: Main display screen for temperature readings and pressure readings

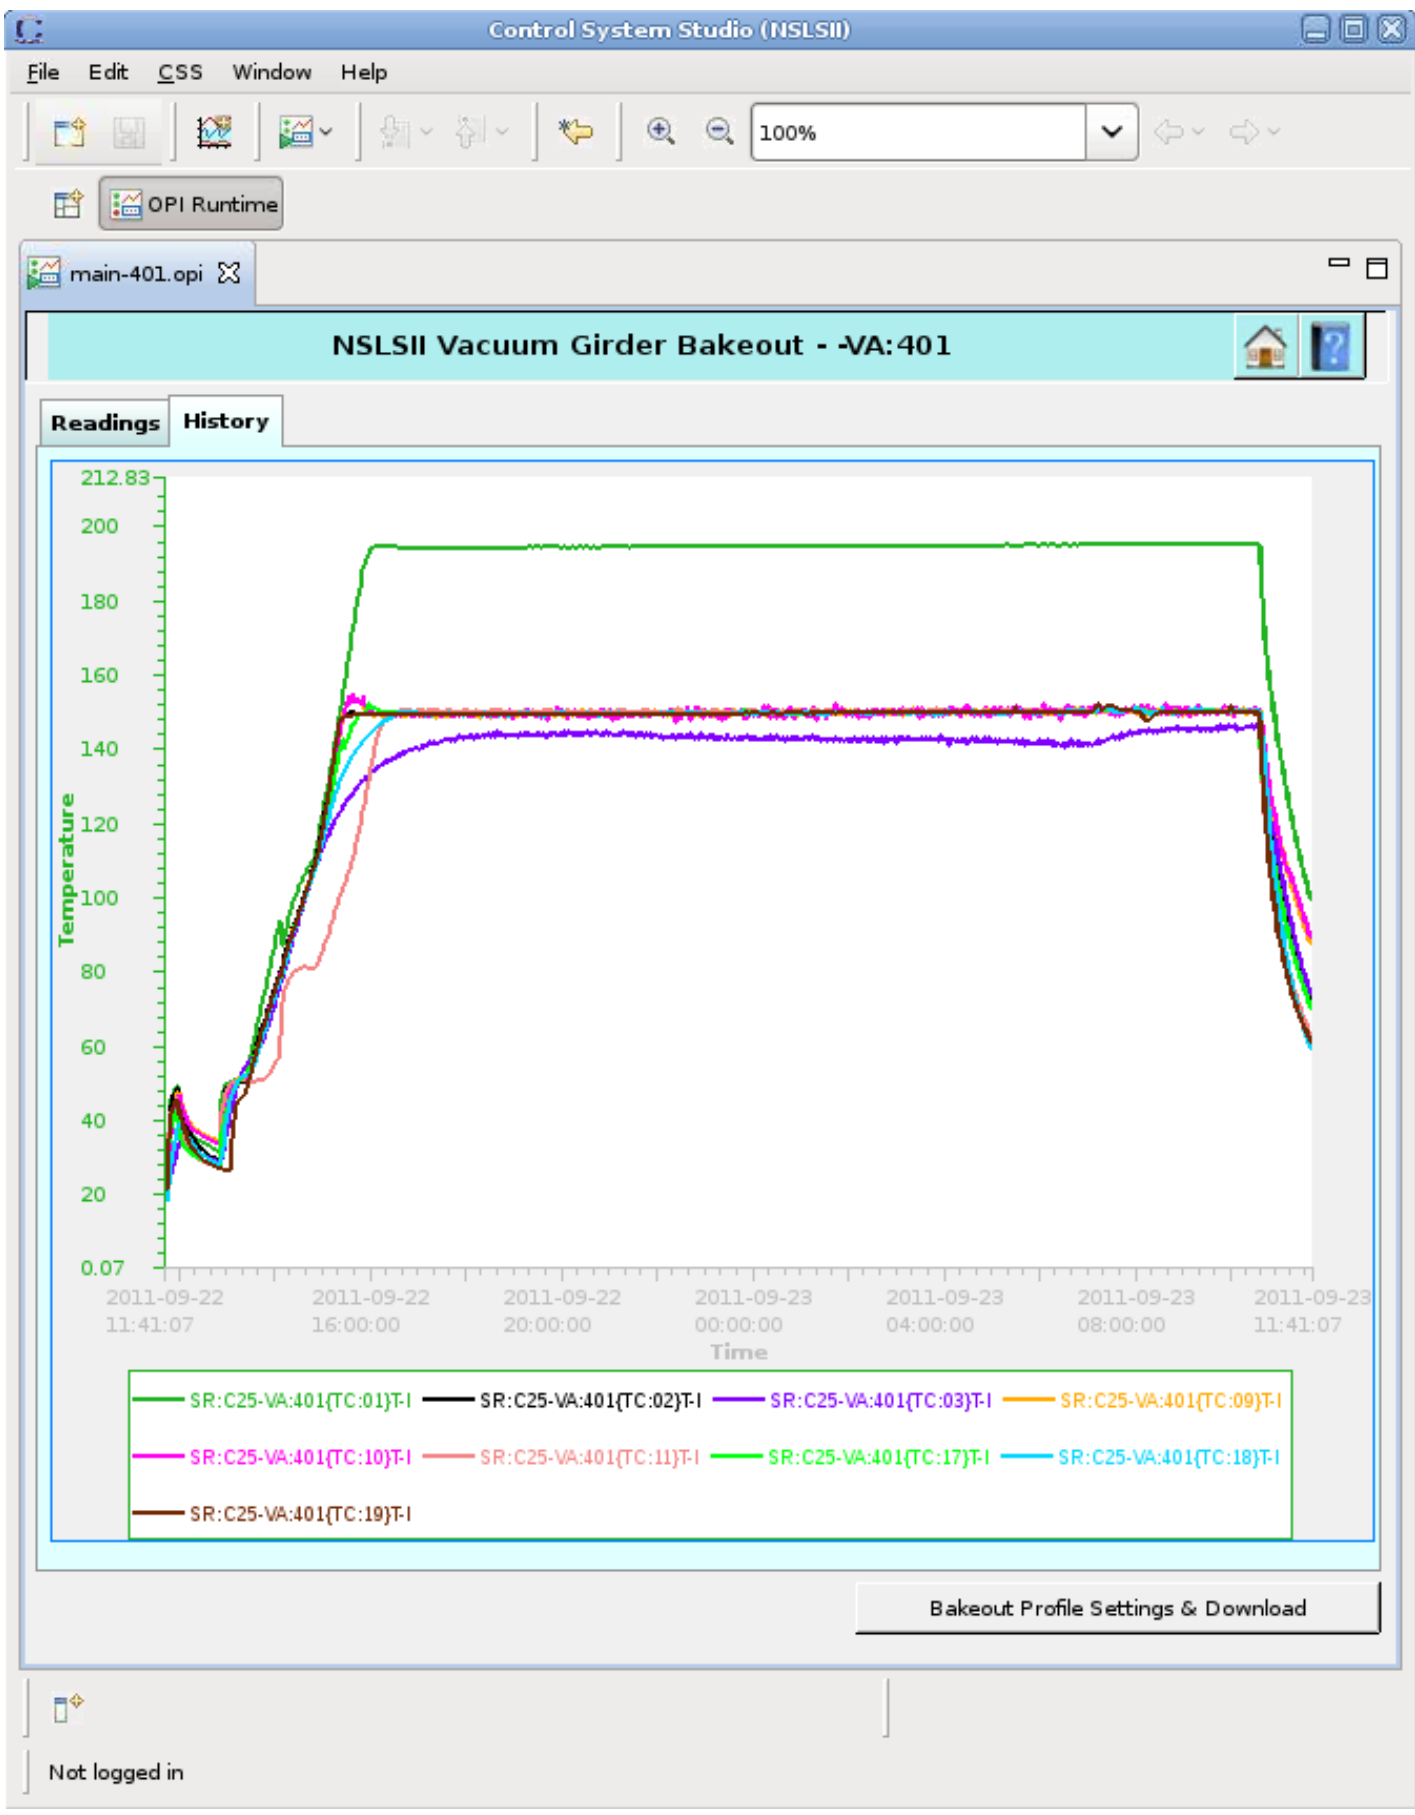


Figure 4: Historical data with data browser readings

Data Logging

Channel Archiver is used to log all temperatures, ion pump current, and gauge pressure readings. A low-cost Acer Aspire Revo series PC is used as the data server. This PC also works as the gateway between campus computers and I/O controllers. Data browser provides an easy way to review and analyze logged data. Figure 4 shows the historical view of the temperature readings.

Interlock

The interlock is provided by a MKS 937B gauge controller. A Cold Cathode and Pirani gauge pair provides an adjustable setpoint that is hardwired to each of the vacuum controllers including the ion pump controller, tsp, bakeout cart and NEG controllers. The setpoint status can be monitored via the serial communication port of the gauge controller.

SUMMARY

To date, 4 fully assembled girder chambers have been processed and successfully baked. The girder bakeout control system has worked well. We're still learning from the girder bakeout and intend on improving system performance.