

NUMERICAL MODELING AND DEVELOPMENT OF THE PROTOTYPE OF THE BRAGG PEAK POSITION DETECTOR WORKING IN REAL TIME MODE FOR HADRON THERAPY FACILITIES PROMETHEUS

A.A. Pryanichnikov, M.A. Belikhin, A.S. Simakov, P.N. Lebedev Physical Institute of the Russian Academy of Sciences, Physical Technical Center (PhTC LPI RAS), Protvino, Russia
 I.I. Degtyarev, F.N. Novoskoltsev, E.V. Altukhova, Yu. V. Altukhov, R. Yu. Sinyukov, Institute for High Energy Physics of the National Research Centre “Kurchatov Institute” (NRC KI – IHEP), Protvino, Russia

Abstract

The purpose of this research was precision statistical simulation of multi-particle radiation transport using a realistic 3D model of clinical setup prototype and the systems of slot-hole collimators for on-line monitoring of Bragg-peak position at a proton therapy complex “Prometheus” to define of an available detecting accuracy and the choice of its optimum parameters. Numerical simulation of the experiments was carried out based on the RTS&T [1,2] high-precision radiation transport software package using files of evaluated nuclear data from ENDF/B VIII.0 library [5].

INTRODUCTION

Hadron therapy using the pencil beam scanning technique is the most accurate kind of remote radiation therapy. High accuracy is due to the fundamental physical property of protons and ions - to stop in the tissue at a certain depth, the so-called Bragg peak. This is why hadron therapy is used to treat critical organs, in particular the brain. However, accuracy in proton delivery is limited by uncertainty surrounding the hadron beam range. The detector considered in this paper is able to determine the hadron ranges by prompt gamma radiation [3] in real time mode. Basically this detector is planed to use with the proton therapy complex “Prometheus” [4].

NUMERICAL SIMULATION

Figure 1 illustrates the linear energy deposition and production of prompt γ -rays in inelastic nuclear interactions of primary protons in the water phantom. Definition of Bragg-peak position Z_p comes down to a problem of longitudinal (along a beam direction) coordinates definition for a spatial point Z_γ in which density of prompt γ -rays production decreases practically to zero:

$$Z_p = Z_\gamma - \Delta Z, \text{ where } \Delta Z - \text{calculated coefficient.}$$

The elementary diagram for basic elements of calculated system (the water phantom, collimator system, plate of scintillation detectors) is shown on fig. 2.

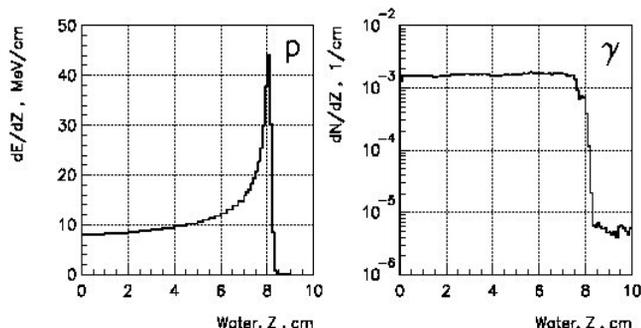


Figure 1: The deep distribution of energy deposition and the density of prompt γ -rays production from the primary proton beam with an energy of 100 MeV in the water phantom.

The prompt γ -rays flux is formed by the system of the slot-hole collimators made of heavy alloys of the residence permit brands (tungsten-nickel-iron, WNiFe). The water phantom is cylinder of 20 cm long and with a radius of 10 cm in which center the proton beam with energy of 100 MeV is dumped. The distance along a beam from a front edge of the collimator to the phantom is 19.2 cm.

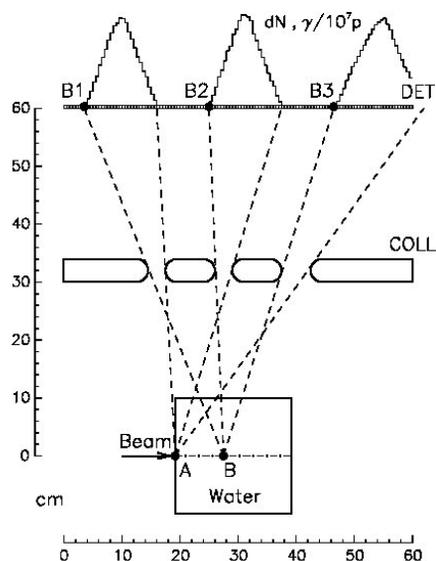


Figure 2: The design scheme of the clinical setup (side view).

Content from this work may be used under the terms of the CC BY 3.0 licence © 2018). Any distribution of this work must maintain attribution to the author(s), title of the work, publisher, and DOI.

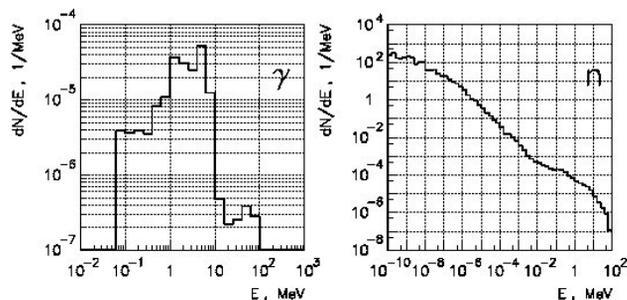


Figure 3: Energy distributions of prompt γ -rays and neutrons from a primary proton beam with an energy of 100 MeV.

This distance was chosen so that the longitudinal coordinate (8.3 cm) of a point in which the calculated density of prompt γ -rays production in water could already be considered equal to zero (fig. 2) was exactly in the center of the second crack of the collimator (19.2 + 8.3 = 27.5 cm). Apart from 30 to 34 cm from an axis of a beam the collimator 4 cm thick and cross sectional dimensions 60×60 cm² is located. In the collimator, there are transversal slits with rounded edges. Width of slits along a beam is 3, 3 and 5 cm. The distance along a beam from the beginning of the collimator to the center of slits are 16, 27.5 and 40 cm respectively. At a distance of 60 cm from the beam axis, a γ -rays detector with transverse dimensions also 60×60 cm² is located strictly above the collimator, showed in Fig. 2. The upper part of the figure shows of prompt γ -rays distribution in the case of black collimator and without taking into account the neutron background (the distributions presented in Fig. 4). Prompt γ -rays are produced in the water phantom at points whose longitudinal coordinates are in the interval from zero (point A) to 8.3 cm (point B).

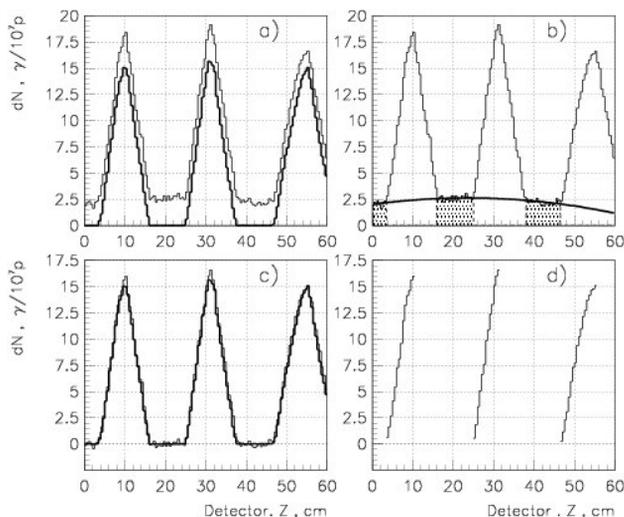


Figure 4: The distribution along the longitudinal coordinate of prompt γ -rays intensity at the detector. Idealized distribution (thick line) - without taking into account the contribution of neutrons using absolutely black collimators; realistic distribution (thin line) - taking into account the neutron background and realistic WNiFe-collimators): a) - realistic and idealized distribution; b) definition of the

background for a realistic distribution; c) realistic without background and idealized distribution. d) the left parts of the peaks of a realistic distribution without background.

The detector is assembled from scintillation plates with a width of 60 cm, a beam length of 0.5 cm and a thickness of 5 cm. Thus, the detector represents a lattice from 120 plates with a step of 5 mm and does not distinguish γ -rays with different transverse coordinates. On fig. 3 the energy distributions for γ -rays and neutrons on the detector plates are presented. Taking into account these distributions (Fig. 5) the optimum type of a scintillator was found - BGO crystal scintillator.

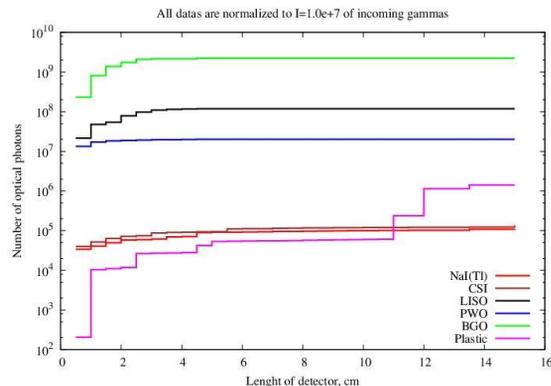


Figure 5: The light output of the detecting element of the matrix, made of different types of scintillator.

RESULTS

To determine the error of the longitudinal Bragg peak monitoring, a series of 24 calculations was performed using different sequences of pseudo-random numbers to construct trajectories of particles in the calculation system. When using 3 slits, the RMS-error in determining the longitudinal coordinate was 1.5 mm.

REFERENCES

- [1] I.I. Degtyarev, F.N. Novoskoltsev, O.A. Liashenko, E.V. Gulina, L.V. Morozova, RTS&T 2014 Code Status, Nuclear Energy and Technology 1(2015) 222-225.
- [2] A.I. Blokhin, I.I. Degtyarev, A.E. Lkhovitskii, M.A. Maslov, and I.A. Yazynin. RTS&T Monte Carlo Code (Facilities and Computation Methods), in.: SARE-3 Workshop, KEK, Tsukuba, Japan, May 1997; INDC (CCP)-426.
- [3] C.-H. Min, C. H. Kim, M.-Y. Youn and J.-W. Kim, Prompt gamma measurements for locating the dose falloff region in the proton therapy, Appl. Phys. Lett., 2006, v. 89, p.183.
- [4] A.A. Pryanichnikov, V.V. Sokunov, A.E. Shemyakov, "Some results of the clinical use of the proton therapy complex "Prometheus"", In.: 12th International Scientific Workshop in Memory of Professor V.P. Sarantsev "Problems of Colliders and Charged Particle Accelerators", 2017.
- [5] A.A. Pryanichnikov et al., Verification of the world evaluated nuclear data libraries on the basis of integral experiments using the RTS&T code system, Problems of Atomic Science and Technology. Series: Nuclear and Reactor Constants, 1, p. 127, (2018)